

Table 4. Confidence intervals (95%) for the amount of moisture lost to evapotranspiration after irrigation is withheld before bluegrass selections reach 75, 50, and 25% green cover. Selections are ranked based on their ET₅₀ values.

Rank	Selection	ET ₇₅	ET ₅₀	ET ₂₅
1.	Mallard	4.224 to 4.866	5.828 to 6.582	7.126 to 8.604
2.	AKB2543	4.374 to 5.467	5.585 to 6.726	6.272 to 8.510
3.	Midnight	4.219 to 4.635	5.496 to 5.836	6.593 to 7.216
4.	AKB2274	3.713 to 4.630	5.018 to 5.715	5.967 to 7.158
5.	AKB2260	3.664 to 4.771	4.924 to 5.754	5.774 to 7.148
6.	AKB2192	3.410 to 4.358	4.964 to 5.706	6.111 to 7.462
7.	Ridgeline	3.718 to 4.273	5.097 to 5.522	6.251 to 6.996
8.	AKB2242	3.663 to 4.189	5.073 to 5.474	6.267 to 6.973
9.	Diva	3.422 to 4.624	4.764 to 5.661	5.657 to 7.148
10.	AKB2150	3.366 to 4.575	4.748 to 5.653	5.670 to 7.191
11.	A05-325	3.614 to 4.262	4.952 to 5.437	6.040 to 6.861
12.	AKB2306	3.426 to 4.152	4.899 to 5.444	6.076 to 7.032
13.	AKB1925	3.806 to 4.293	4.989 to 5.351	5.999 to 6.582
14.	AKB1908	3.723 to 4.299	4.947 to 5.376	5.964 to 6.660
15.	AKB2512	3.420 to 4.300	4.795 to 5.448	5.835 to 6.931
16.	AKB2094	3.572 to 3.879	4.985 to 5.214	6.276 to 6.671
17.	AKB2035	3.039 to 4.041	4.711 to 5.457	5.957 to 7.302
18.	AKB2404	3.361 to 4.377	4.703 to 5.454	5.671 to 6.904
19.	AKB1887	3.372 to 3.939	4.868 to 5.287	6.132 to 6.866
20.	AKB2162	3.520 to 4.139	4.821 to 5.277	5.894 to 6.643
21.	AKB2538	3.275 to 4.102	4.714 to 5.320	5.833 to 6.858
22.	AKB2262	3.056 to 4.621	4.441 to 5.591	5.266 to 7.121
23.	AKB2563	3.454 to 3.892	4.820 to 5.140	6.019 to 6.555
24.	AKB2202	3.324 to 3.972	4.741 to 5.213	5.909 to 6.704
25.	AKB2203	3.575 to 4.241	4.724 to 5.217	5.653 to 6.413
26.	AKB1892	3.159 to 3.798	4.681 to 5.142	5.948 to 6.740
27.	AKB1944	2.622 to 4.134	4.362 to 5.451	5.478 to 7.392
28.	AKB1869	3.215 to 3.926	4.633 to 5.146	5.782 to 6.634
29.	America	3.373 to 4.087	4.603 to 5.124	5.588 to 6.405
30.	AKB1998	2.805 to 3.970	4.432 to 5.264	5.595 to 7.023
31.	AKB2460	3.012 to 3.805	4.551 to 5.117	5.779 to 6.740
32.	Baron	3.045 to 4.043	4.453 to 5.169	5.497 to 6.659
33.	AKB1882	2.728 to 4.208	4.265 to 5.321	5.249 to 6.987
34.	AKB2254	2.603 to 3.909	4.295 to 5.213	5.466 to 7.038
35.	AKB2201	2.891 to 3.560	4.467 to 4.934	5.781 to 6.571
36.	AKB1985	3.150 to 4.014	4.356 to 4.982	5.277 to 6.237
37.	AKB2325	2.502 to 3.489	4.314 to 4.993	5.718 to 6.908
38.	AKB1912	2.769 to 3.627	4.323 to 4.918	5.551 to 6.535
39.	AKB2363	2.038 to 3.578	4.096 to 5.144	5.489 to 7.375
40.	AKB2399	3.224 to 3.831	4.397 to 4.835	5.370 to 6.040
41.	AKB1884	3.052 to 3.827	4.311 to 4.863	5.306 to 6.161
42.	AKB2119	3.261 to 3.723	4.421 to 4.752	5.427 to 5.935
43.	AKB2226	3.343 to 3.879	4.388 to 4.780	5.261 to 5.853
44.	AKB2209	2.911 to 3.643	4.321 to 4.832	5.466 to 6.284
45.	AKB2551	3.279 to 3.783	4.334 to 4.699	5.225 to 5.777

46.	AKB2403	3.186 to 3.819	4.285 to 4.742	5.179 to 5.871
47.	AKB2350	3.548 to 3.725	4.448 to 4.577	5.290 to 5.486
48.	AKB2352	2.982 to 3.549	4.284 to 4.680	5.390 to 6.007
49.	AKB2313	2.685 to 3.725	4.114 to 4.835	5.176 to 6.312
50.	Brooklawn	2.878 to 3.783	4.152 to 4.790	5.121 to 6.102
51.	AKB2118	3.150 to 3.555	4.316 to 4.603	5.346 to 5.785
52.	AKB2239	3.196 to 3.705	4.275 to 4.640	5.188 to 5.740
53.	AKB2252	3.060 to 3.694	4.224 to 4.674	5.180 to 5.864
54.	AKB2532	3.073 to 3.574	4.235 to 4.589	5.232 to 5.770
55.	AKB2194	2.663 to 3.815	4.009 to 4.813	4.964 to 6.202
56.	AKB1971	2.847 to 3.819	4.029 to 4.716	4.893 to 5.932
57.	AKB2413	2.961 to 3.772	4.084 to 4.659	4.942 to 5.810
58.	AKB2426	2.989 to 3.561	4.168 to 4.570	5.158 to 5.768
59.	AKB2373	2.882 to 3.674	4.064 to 4.621	4.986 to 5.828
60.	AKB2181	2.969 to 3.531	4.142 to 4.534	5.128 to 5.724
61.	AKB2217	3.104 to 3.678	4.120 to 4.527	4.949 to 5.562
62.	AKB2335	2.447 to 3.555	3.930 to 4.681	5.023 to 6.197
63.	AKB2107	2.734 to 3.706	3.958 to 4.636	4.862 to 5.886
64.	AKB2392	3.008 to 3.447	4.079 to 4.385	5.006 to 5.465
65.	AKB2285	2.342 to 3.300	3.888 to 4.524	5.091 to 6.090
66.	AKB2310	2.893 to 3.526	3.984 to 4.425	4.870 to 5.529
67.	AKB2124	2.446 to 3.830	3.719 to 4.675	4.539 to 5.975
68.	AKB2555	2.837 to 3.375	3.985 to 4.355	4.956 to 5.512
69.	AKB2305	2.954 to 3.566	3.948 to 4.372	4.745 to 5.376
70.	AKB2295	2.582 to 3.351	3.898 to 4.419	4.955 to 5.746
71.	AKB2149	2.595 to 3.248	3.933 to 4.373	5.050 to 5.720
72.	AKB2291	2.222 to 3.840	3.573 to 4.679	4.392 to 6.049
73.	AKB2457	2.921 to 3.284	3.995 to 4.246	4.952 to 5.325
74.	AKB2120	2.619 to 3.188	3.895 to 4.279	4.981 to 5.559
75.	AKB2234	2.628 to 3.359	3.758 to 4.256	4.654 to 5.388
76.	AKB1902	2.600 to 3.472	3.692 to 4.286	4.506 to 5.378
77.	AKB2213	2.740 to 3.447	3.744 to 4.227	4.525 to 5.228
78.	AKB2235	2.138 to 2.903	3.729 to 4.222	5.051 to 5.812
79.	AKB2151	2.800 to 3.365	3.668 to 4.054	4.372 to 4.907
80.	AKB2436	2.775 to 3.217	3.695 to 3.997	4.482 to 4.909
81.	AKB2510	2.524 to 3.056	3.603 to 3.960	4.516 to 5.031
82.	AKB2427	2.676 to 3.238	3.574 to 3.961	4.310 to 4.846
83.	AKB2282	2.707 to 3.064	3.643 to 3.887	4.472 to 4.816
84.	AKB2397	2.243 to 3.031	3.461 to 3.978	4.427 to 5.177
85.	AKB2174	1.565 to 3.357	3.133 to 4.285	4.116 to 5.799
86.	AKB2438	2.610 to 3.088	3.500 to 3.831	4.254 to 4.710
87.	AKB2358	1.796 to 2.956	3.143 to 3.883	4.123 to 5.177
88.	AKB2221	1.754 to 3.241	2.996 to 3.967	3.779 to 5.152
89.	AKB2344	1.685 to 2.386	3.159 to 3.596	4.413 to 5.026
90.	AKB2256	1.166 to 2.451	2.809 to 3.604	4.060 to 5.148
91.	AKB2122	1.241 to 2.998	2.581 to 3.669	3.387 to 4.873
92.	AKB2218	1.154 to 2.769	2.590 to 3.584	3.548 to 4.878

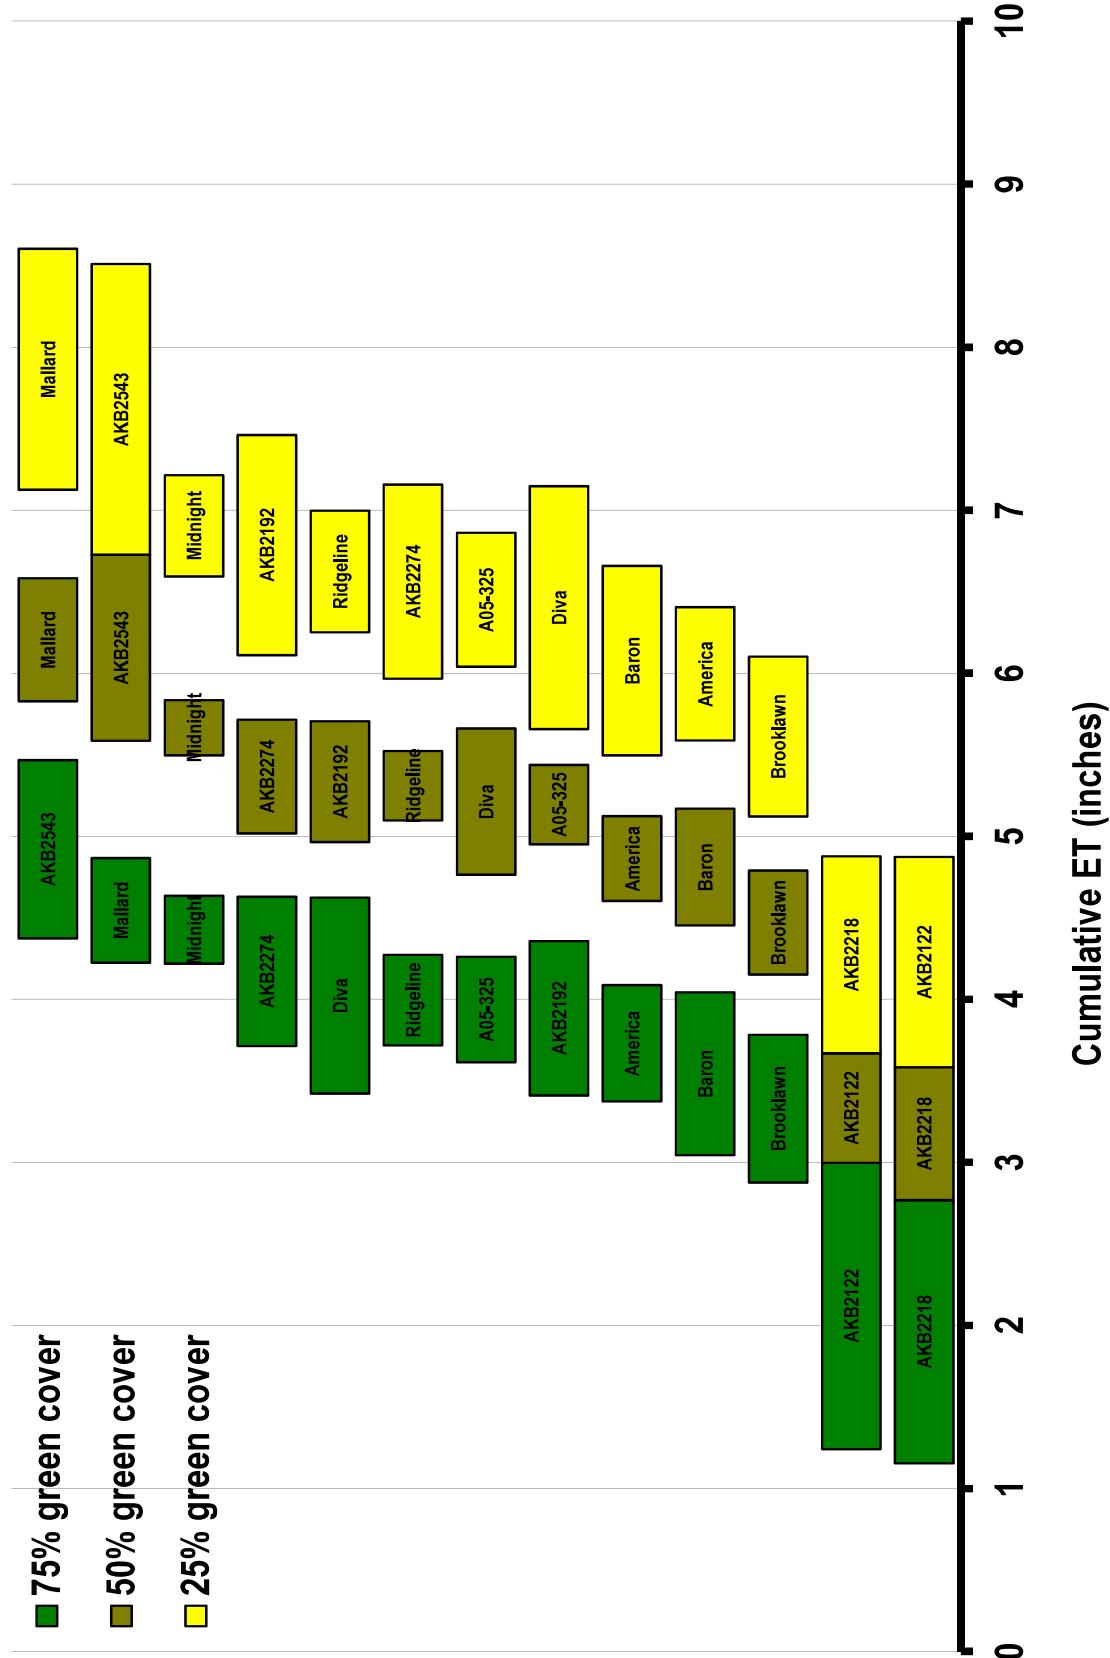


Figure 4. Confidence intervals (95%) for the amount of moisture lost to evapotranspiration after irrigation is withheld before selections reach 75, 50, and 25% green cover.