


**Table 2. Confidence intervals (95%) for the amount of moisture lost to evapotranspiration after irrigation is withheld before 48 entries from data set 11ALP2 reach 75, 50, and 25% green cover. Entries are ranked based on their ET<sub>50</sub> values.**

Rank	Selection	ET <sub>75</sub>	ET <sub>50</sub>	ET <sub>25</sub>
1.	APR2225	6.493 to 7.127	7.867 to 8.309	9.060 to 9.673
2.	APR2186	6.322 to 7.243	7.746 to 8.390	8.908 to 9.801
3.	APR2535	6.271 to 6.863	7.612 to 8.032	8.790 to 9.363
4.	APR2436	6.500 to 6.981	7.627 to 7.970	8.628 to 9.084
5.	APR2462	5.478 to 6.551	7.246 to 8.017	8.694 to 9.805
6.	APR2536	6.115 to 6.656	7.427 to 7.816	8.593 to 9.121
7.	APR2448	5.759 to 6.430	7.367 to 7.849	8.781 to 9.463
8.	APR2450	6.144 to 6.716	7.382 to 7.795	8.469 to 9.024
9.	APR2198	6.173 to 6.688	7.383 to 7.755	8.457 to 8.956
10.	APR2463	6.088 to 6.534	7.393 to 7.716	8.579 to 9.016
11.	APR2451	5.952 to 6.540	7.334 to 7.760	8.557 to 9.138
12.	APR2533	5.943 to 6.458	7.274 to 7.648	8.468 to 8.977
13.	APR2464	5.119 to 6.406	6.954 to 7.886	8.409 to 9.747
14.	APR2455	5.803 to 6.374	7.134 to 7.551	8.312 to 8.881
15.	APR2466	5.897 to 6.340	7.179 to 7.504	8.343 to 8.784
16.	APR2212	5.937 to 6.447	7.149 to 7.524	8.227 to 8.733
17.	APR2201	5.785 to 6.298	7.143 to 7.519	8.364 to 8.877
18.	APR2105	5.817 to 6.436	7.102 to 7.556	8.222 to 8.838
19.	APR2447	5.074 to 6.243	6.895 to 7.744	8.372 to 9.589
20.	APR2106	5.662 to 6.213	7.110 to 7.513	8.407 to 8.963
21.	Manhattan II	5.960 to 6.509	7.108 to 7.512	8.113 to 8.657
22.	APR2467	5.768 to 6.318	7.099 to 7.503	8.283 to 8.833
23.	APR2437	5.821 to 6.347	7.102 to 7.488	8.243 to 8.768
24.	APR2104	5.676 to 6.137	7.005 to 7.345	8.212 to 8.677
25.	Phenom	5.549 to 6.183	6.940 to 7.407	8.160 to 8.802
26.	APR2154	5.584 to 6.192	6.888 to 7.338	8.030 to 8.646
27.	APR2460	5.358 to 5.995	6.828 to 7.298	8.124 to 8.775
28.	APR2461	5.421 to 6.016	6.835 to 7.276	8.087 to 8.696
29.	APR2465	5.545 to 6.018	6.862 to 7.213	8.052 to 8.535
30.	APR2440	5.576 to 6.063	6.850 to 7.213	7.995 to 8.492
31.	APR2208	5.495 to 6.106	6.801 to 7.256	7.945 to 8.569
32.	APR2459	5.449 to 5.981	6.830 to 7.224	8.067 to 8.611
33.	APR2280	5.579 to 5.994	6.842 to 7.151	7.994 to 8.419
34.	APR2438	5.403 to 6.063	6.747 to 7.237	7.913 to 8.589
35.	APR2534	5.563 to 6.026	6.807 to 7.153	7.928 to 8.404
36.	Pop (APR2142)	5.396 to 6.019	6.708 to 7.173	7.853 to 8.494
37.	APR2456	5.317 to 6.145	6.624 to 7.242	7.709 to 8.561
38.	APR2453	5.580 to 6.039	6.739 to 7.085	7.777 to 8.252
39.	Radiance	5.521 to 6.018	6.700 to 7.073	7.746 to 8.261

40.	APR2149	5.168 to 5.766	6.563 to 7.010	7.796 to 8.418
41.	APR2458	5.509 to 5.900	6.626 to 6.922	7.638 to 8.049
42.	Integra II	5.097 to 5.671	6.555 to 6.982	7.854 to 8.452
43.	APR2452	5.340 to 5.733	6.598 to 6.893	7.748 to 8.160
44.	APR2457	5.134 to 5.745	6.504 to 6.961	7.706 to 8.344
45.	APR2532	4.937 to 5.591	6.464 to 6.950	7.809 to 8.492
46.	APR2449	4.974 to 5.613	6.403 to 6.880	7.654 to 8.323
47.	APR2439	4.909 to 5.656	6.281 to 6.842	7.446 to 8.235
48.	APR2454	5.217 to 5.580	6.400 to 6.674	7.482 to 7.869

---

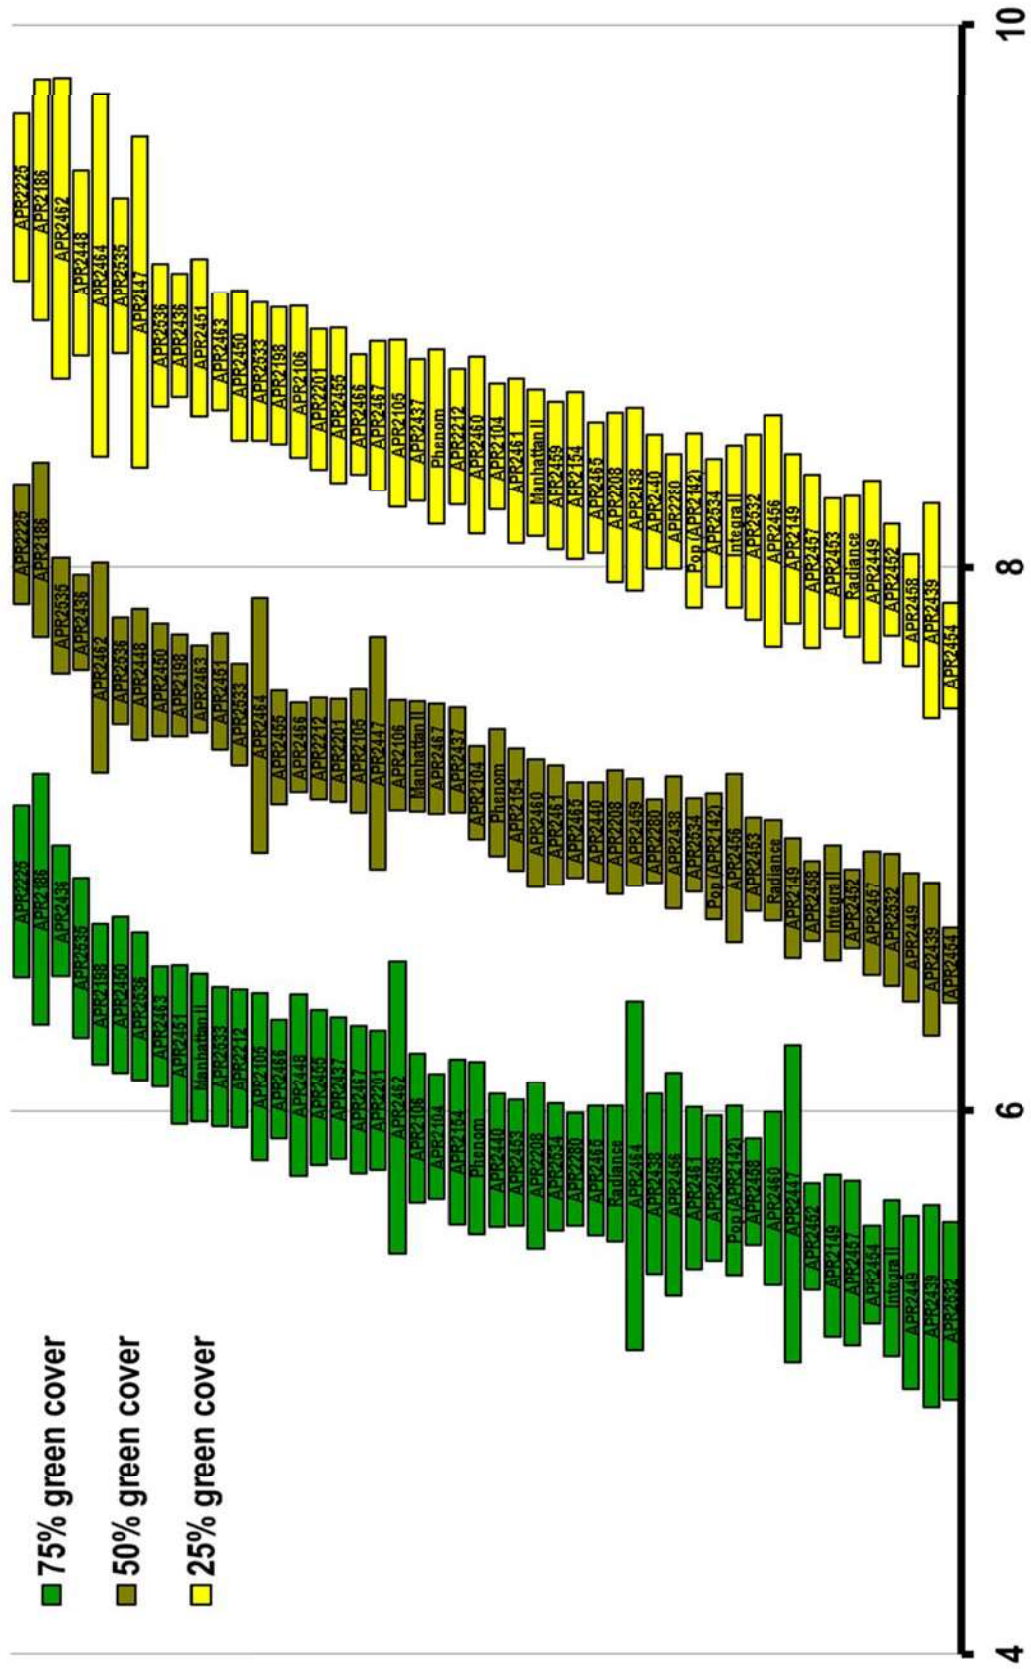

Cumulative ET (inches)

Figure 2. Confidence intervals (95%) for the amount of moisture lost to evapotranspiration after irrigation is withheld before 48 entries from data set 11ALP2 reach 75, 50, and 25% green cover.