

Table 2. Confidence intervals (95%) for the amount of moisture lost to evapotranspiration after irrigation is withheld before 38 entries from data set 11AFA1 reach 75, 50, and 25% green cover. Entries are ranked based on their ET₅₀ values.

Rank	Entry	ET ₇₅	ET ₅₀	ET ₂₅
1.	ATF1730	9.203 to 10.04	12.62 to 13.22	15.70 to 16.74
2.	ATF1736	8.789 to 9.725	12.15 to 12.82	15.17 to 16.26
3.	ATF1617	8.101 to 9.488	11.90 to 12.90	15.17 to 16.86
4.	ATF1616	8.365 to 9.767	11.86 to 12.85	14.83 to 16.46
5.	ATF1485	8.730 to 9.829	11.97 to 12.74	14.81 to 16.05
6.	ATF1739	8.194 to 9.095	11.98 to 12.63	15.42 to 16.52
7.	ATF1729	8.740 to 9.789	11.91 to 12.64	14.71 to 15.87
8.	ATF1722R	8.561 to 9.263	11.95 to 12.45	15.09 to 15.89
9.	Falcon IV	8.625 to 9.518	11.83 to 12.45	14.71 to 15.70
10.	ATF1738	7.838 to 9.613	11.47 to 12.72	14.45 to 16.48
11.	ATF1434	8.477 to 9.278	11.80 to 12.36	14.84 to 15.74
12.	ATF1458	8.011 to 9.028	11.56 to 12.28	14.75 to 15.90
13.	ATF1722S	8.258 to 9.243	11.47 to 12.15	14.34 to 15.39
14.	ATF1426	8.172 to 8.767	11.55 to 11.97	14.72 to 15.38
15.	ATF1622	7.989 to 8.752	11.22 to 11.75	14.19 to 15.00
16.	ATF1732	8.284 to 8.769	11.29 to 11.62	14.13 to 14.64
17.	ATF1728	8.007 to 8.701	11.11 to 11.59	13.98 to 14.70
18.	ATF1707	7.994 to 8.751	11.01 to 11.53	13.78 to 14.55
19.	ATF1492	7.869 to 8.681	10.94 to 11.51	13.76 to 14.59
20.	ATF1402	7.282 to 8.498	10.76 to 11.61	13.83 to 15.12
21.	ATF1724R	7.447 to 8.420	10.83 to 11.51	13.90 to 14.92
22.	ATF1706	7.247 to 8.109	10.69 to 11.29	13.85 to 14.76
23.	ATF1740	7.846 to 8.684	10.67 to 11.25	13.25 to 14.08
24.	ATF1734	7.528 to 8.166	10.68 to 11.12	13.63 to 14.28
25.	ATF1731	7.915 to 8.530	10.67 to 11.09	13.23 to 13.84
26.	ATF1735	7.634 to 8.619	10.54 to 11.22	13.15 to 14.13
27.	ATF1723S	6.460 to 8.596	10.09 to 11.57	13.02 to 15.24
28.	ATF1701	8.097 to 8.667	10.62 to 11.02	12.99 to 13.54
29.	ATF1705	7.259 to 8.168	10.48 to 11.11	13.41 to 14.33
30.	ATF1733	7.131 to 8.095	10.34 to 11.01	13.25 to 14.22
31.	ATF1702	7.207 to 8.367	10.24 to 11.05	12.93 to 14.08
32.	ATF1703	7.674 to 8.334	10.39 to 10.85	12.92 to 13.57
33.	ATF1737	7.827 to 8.282	10.39 to 10.71	12.82 to 13.26
34.	ATF1723R	6.972 to 8.000	10.13 to 10.85	12.98 to 14.01
35.	ATF1479	6.632 to 7.734	9.717 to 10.48	12.48 to 13.56
36.	ATF1704	6.379 to 7.355	9.451 to 10.13	12.24 to 13.20
37.	ATF1724S	6.799 to 8.051	9.291 to 10.17	11.44 to 12.63
38.	Crackle	6.024 to 6.732	8.568 to 9.072	10.92 to 11.60

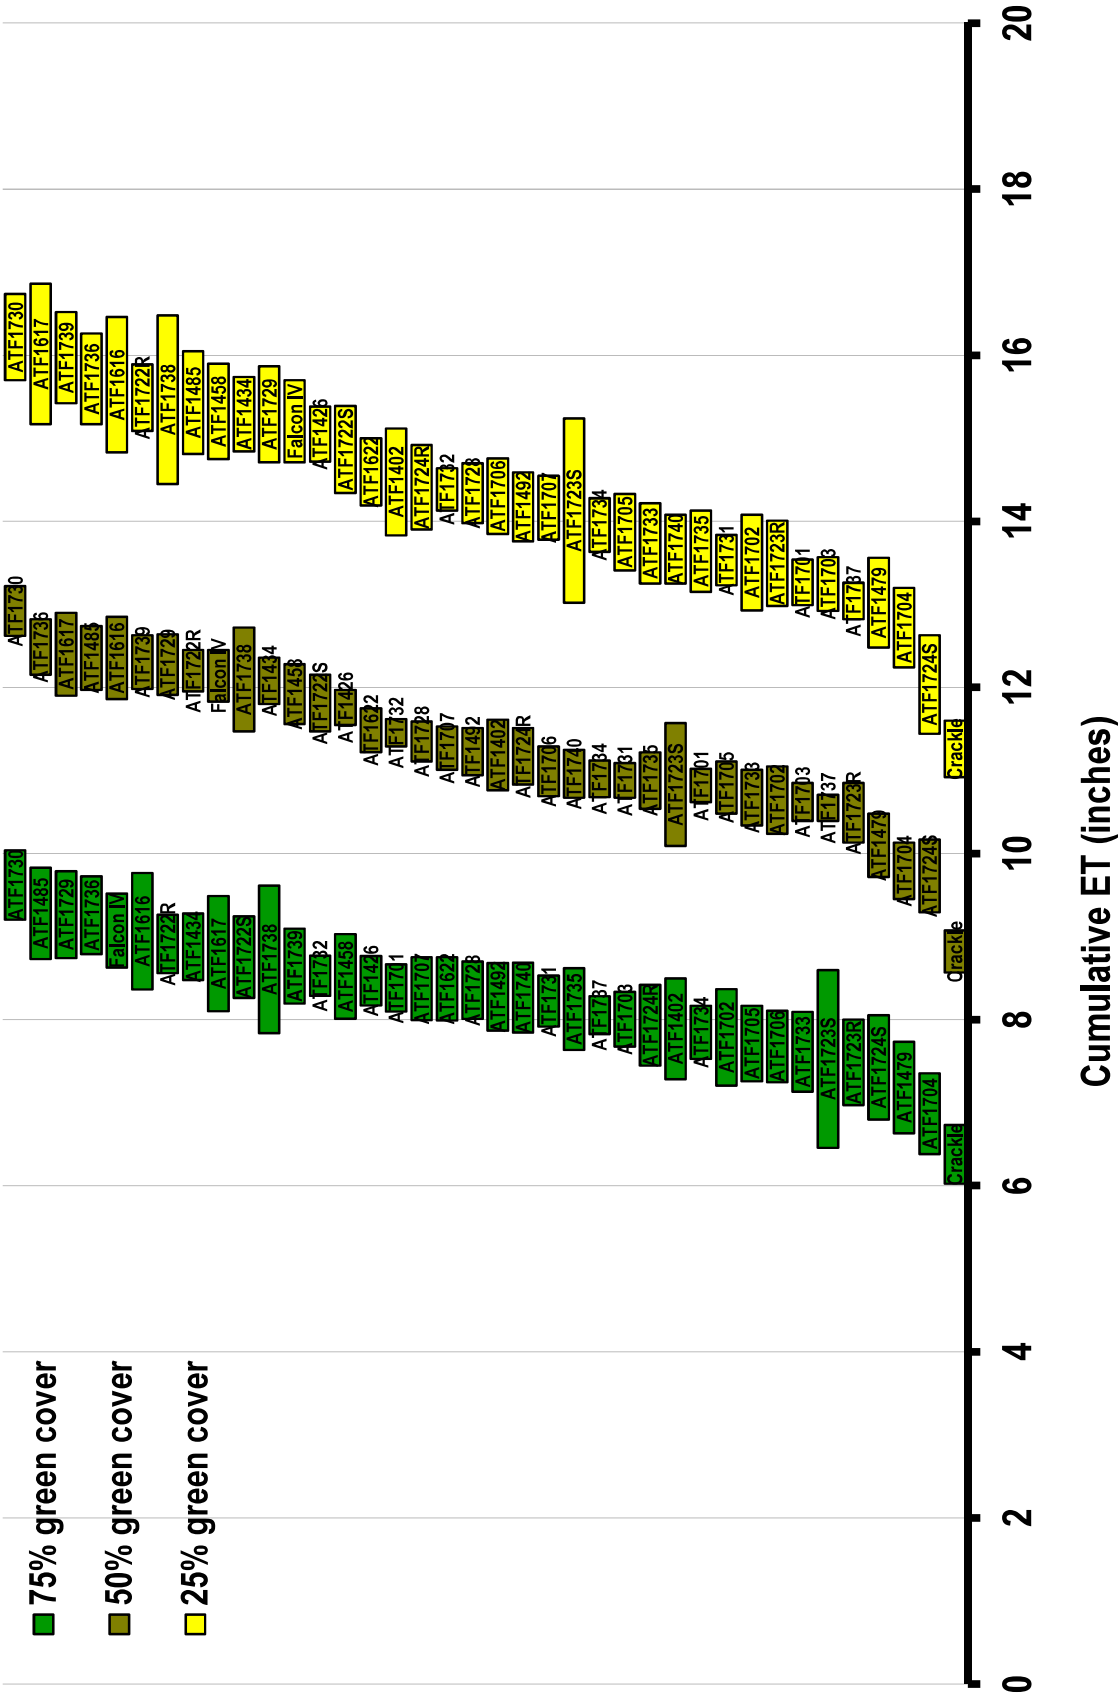


Figure 2. Confidence intervals (95%) for the amount of moisture lost to evapotranspiration after irrigation is withheld before 38 entries from data set 11AFA1 reach 75, 50, and 25% green cover.